



**VORTEX**  
**SUBSEA SOLUTIONS**

# **GAS / LIQUID SAMPLING TOOL**

## **HYDRAULIC OPERATED**

**OPERATIONS MANUAL**

VERSION	SECTION	ISSUE DATE	AUTHOR	DESCRIPTION OF UPDATE
1.0		20 April 2017	JG	First Edition

## VOR-GST-MAN:VER 1.0VST-XX-LP-HYD

Vortex gas sample tool manual version 1.0

### **VORTEX INTERNATIONAL LTD**

27 Parrs Road, RD, New Plymouth 4371, New Zealand  
 Phone/Fax + 64 6 7538102, Mobile + 64 (0) 276 88 53 72  
[vortexdredge.com](http://vortexdredge.com)

# Contents

<b>1.0</b>	<b>INTRODUCTION</b>	<b>2</b>
1.1	Reference Documents	2
1.2	Abbreviations	2
1.3	Contacts	2
<b>2.0</b>	<b>SAFETY</b>	<b>3</b>
2.1	Overview	3
2.2	Risk Assessment	3
2.3	Mechanical	3
<b>3.0</b>	<b>TECHNICAL SPECIFICATIONS</b>	<b>4</b>
3.1	Description	4
3.2	Schematic	5
3.3	Component Particulars	7
<b>4.0</b>	<b>OPERATIONAL PROCEDURES</b>	<b>8</b>
4.1	Pre-dive Checks	8
4.2	Operational Procedure	10
4.3	Recovery to Deck	11
4.4	Gas Sample Removal	12-13
4.5	Post Dive Checks	14-15
<b>5.0</b>	<b>MAINTENANCE &amp; STORAGE</b>	<b>16</b>
5.1	Standard Procedures	16
5.2	Replacement Procedures	16
<b>6.0</b>	<b>APPENDIX AND REFERENCES</b>	<b>17</b>
	Appendix I	
6.1:1	Tool Dimensions and Weights	17
6.2	Spares Contents	18
	Appendix II	
	Suppliers Specifications Sheets	19-29
<b>7.0</b>	<b>GAS TOOL SCHEMATICS</b>	<b>30</b>
<b>8.0</b>	<b>CONTACTS</b>	<b>36</b>

# Introduction

The vortex Hydraulic Mini Gas Sampling tool is designed to capture gas and liquid samples in a subsea environment and recover said samples to the surface in a low pressure state of no more than 14psi (0.96bar) by means of an hydraulic mechanical operated syringe to ingest sample then purge sample into a sample bottle after recovery to surface.

This tool is designed to be deployed from the surface with the syringe bled of air immediately upon entering the water. Sample filling relies on the suck and blow pumping motion created by the syringe and associated relief valves. Sample taken can be discharged or cycled out of the syringe whilst under water if necessary.

## 1.1 REFERENCE DOCUMENTS

See Appendix and references section at the end of this document for certificates and manufacturers data.

## 1.2 ABBREVIATIONS

**PSI:** Pounds per Square Inch

**PPE:** Personnel protective equipment

**JHA:** Job Hazard Analysis

**VST:** Vortex Sample Tool

**LP:** Low Pressure

## 1.3 CONTACTS

For technical queries, comments and feedback contact Vortex Dredge: [goodinjoe@gmail.com](mailto:goodinjoe@gmail.com)

# Safety

## 2.1 OVERVIEW

All local HSE procedures must be followed. Use of PPE should follow guidelines outlined with handling of potential sample. For example hazardous gas samples should have PPE appropriate to mitigate dangers associated with that gas. Safety glasses should be considered minimum requirement irrespective of potential sample. Your safety is your responsibility. Think and plan ahead accordingly.

## 2.2 RISK ASSESSMENT

Consult with local HSE and installation operators to identify best practice steps needed for safe operations. Identify if the task been done and implement lessons learned. JHA, permitting and toolbox talks should preclude all operations.

## 2.3 MECHANICAL

Ensure all fittings and fasteners are secure. Check general condition of tool against images in manual for anything which may indicate potential operational issues.



**REMEMBER, YOUR SAFETY IS YOUR RESPONSIBILITY. THINK AND PLAN AHEAD ACCORDINGLY. IF IN DOUBT, PLEASE ASK.**

# Technical Specifications

## 3.1 DESCRIPTION


To “Suck” the sample into the syringe the operator will function the hydraulic cylinder to draw the piston away from the check valves and draw a vacuum.

To “Blow” the sample out of the tool or into the sample bottle the operator will function the hydraulic cylinder towards the check valves – pushing the sample over the check valve and to atmosphere or into the sample bottle.

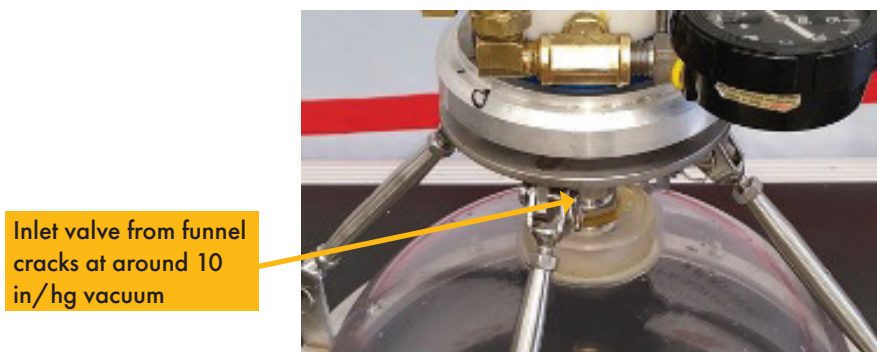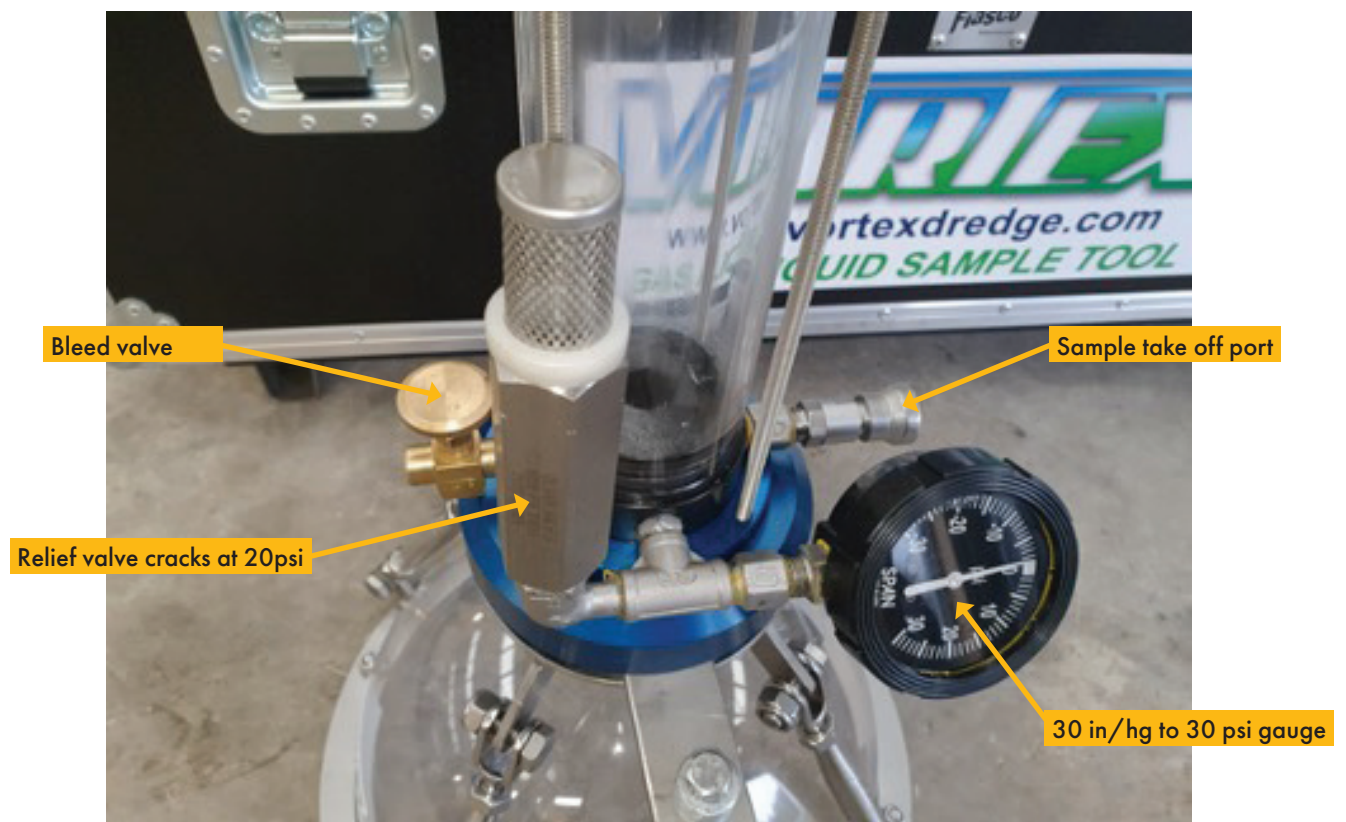

# Technical Specifications

## 3.1 DESCRIPTION SCHEMATICS

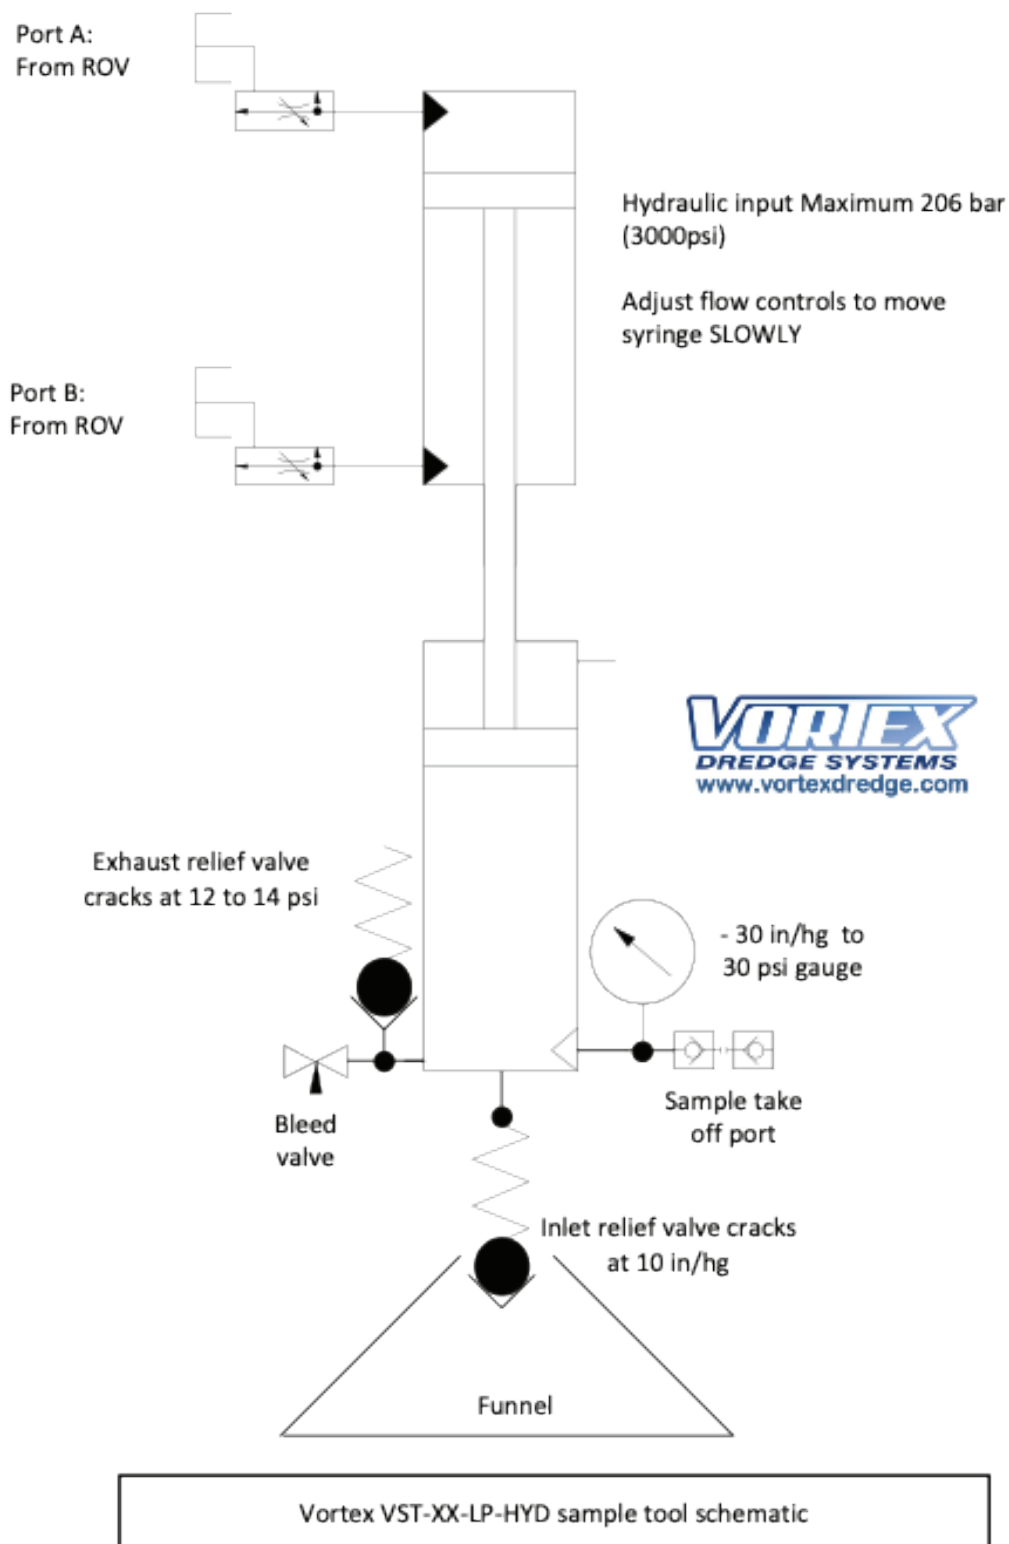

# Technical Specifications

## 3.2 HYDRAULIC CONNECTIONS

Supplied with tool are two -4 jic female swivel, 3000mm long 344bar (5000psi) rated hoses with flow control on each hose.

NOTE: Any questions on hydraulic power supply capabilities from your ROV, please consult the ROV manufacturer.

- Function A = Push or Blow product from syringe.
- Function B = Suck or ingest product into syringe.



# Technical Specifications

## 3.3 COMPONENT PARTICULARS

- Complete tool Weight empty in air = 22lb (10kg)
- Syringe cylinder volume = 0.153 gallon (580 cc)
- Sample bottle volume = 0.264 gallon (1.0 litre)
- Main relief valve setting on syringe = 12psi (0.8 bar)
- Complete tool dimensions = 940 mm (37inch) overall height / tall x 460mm (18 inch) overall width.
- Discharging syringe into sample bottle typically captures 0.268 liter fresh water by volume with exhaust relief set at 20psi.
- Discharging syringe into sample bottle typically captures 0.523 liter of fresh air by volume with exhaust relief set at 20psi.
- Syringe body and end caps material: Acrylic
- Piston material: Acetal
- Piston rings / seals material: Nitrile 50 x 60 x 4
- Piston cap o-rings material : Nitrile N70
- Shipping box dimensions and weight = 88 lb (40kg) L100cm x W50cm x H 50cm.
- Depth rating = 3000 mtr. 9842 foot seawater


# Operation Procedures

## 4.1 PRE DIVE CHECKS

STEP	PROCEDURE DESCRIPTION	CHECK
1	<p>Check hydraulic connection between the tool and ROV. Consult ops manual for voltage figures and connections. See <b>TECHNICAL SPECIFICATIONS</b> in section 3. of this manual.</p> <p>Failure to provide correct pressures and connections as per manual can result in tool cable and motor failure.</p>	
2	<p>Check the piston full stroke in both directions in clear of obstructions.</p> <p>Connect water hose (fresh or salt) to inlet relief valve of tool, open bleed valve CW and purge water through the bleed valve and allow water to pass over the exhaust relief valve to expel any air in the system. Close bleed valve CCW.</p> <p>Launch with the piston at full stroke ready to ingest (piston at rest nearest the two check valves).</p>	
3	<p>Check the bleed valve is closed CCW. Failure to do so can result in insufficient syringe operation and sample being lost to ambient upon ascent.</p>	
4	<p>Check mechanical connections to the ROV are secure.</p>	
5	<p>Check 0 to 30 psi gauge is reading 0 and full of appropriate gauge liquid.</p>	
6	<p>Fit hose and funnel to inlet relief valve – adjust length of hose to suit. Secure funnel where appropriate to view sample being taken.</p>	

# Operation Procedures

## 4.1 PRE DIVE CHECKS (STEPS 2, 3 AND 5)

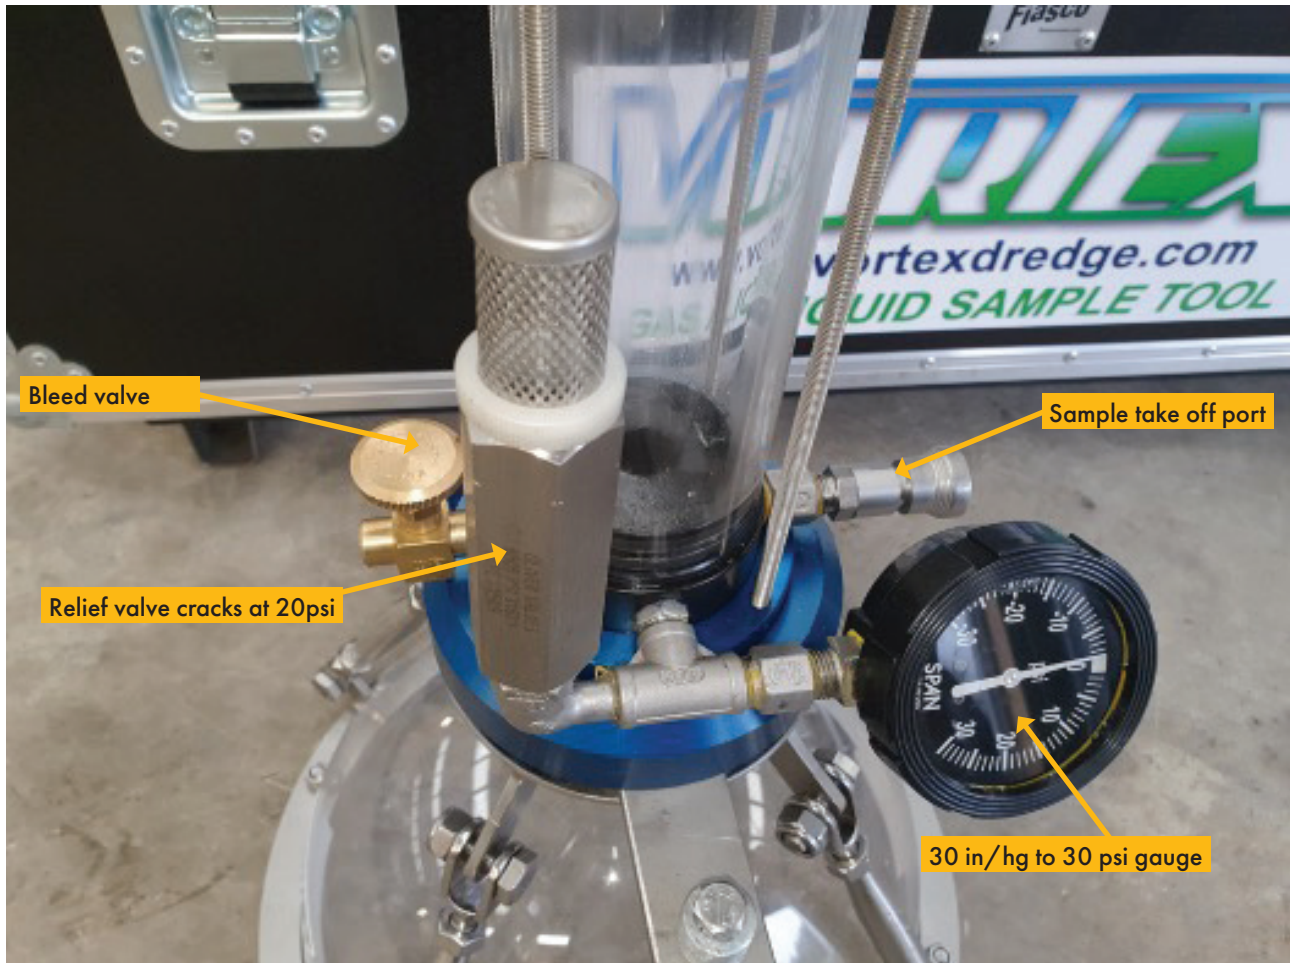

**BLEED VALVE IS CLOCKWISE (CW) TO OPEN  
AND COUNTERCLOCKWISE (CCW) TO CLOSE.  
DO NOT OVER TIGHTEN.**


# Operation Procedures

## 4.2 OPERATION PROCEDURE

STEP	PROCEDURE DESCRIPTION	CHECK
1	Launch with the piston at full stroke ready to ingest (piston at rest nearest the two check valves)	
2	Launch ROV to just below water surface to around 20mtr depth and fully function tool to both ends of stroke in sample cylinder to bleed out any ambient surface air from the system. Stroke tool to rest at full 'blow' position so it is ready to "suck" first sample.	
3	Check the bleed valve is closed CCW. Failure to do so can result in insufficient syringe operation and sample being lost to ambient upon ascent.	
4	Check mechanical connections to the ROV are secure.	

# Operation Procedures

## 4.3 RECOVERY TO DECK

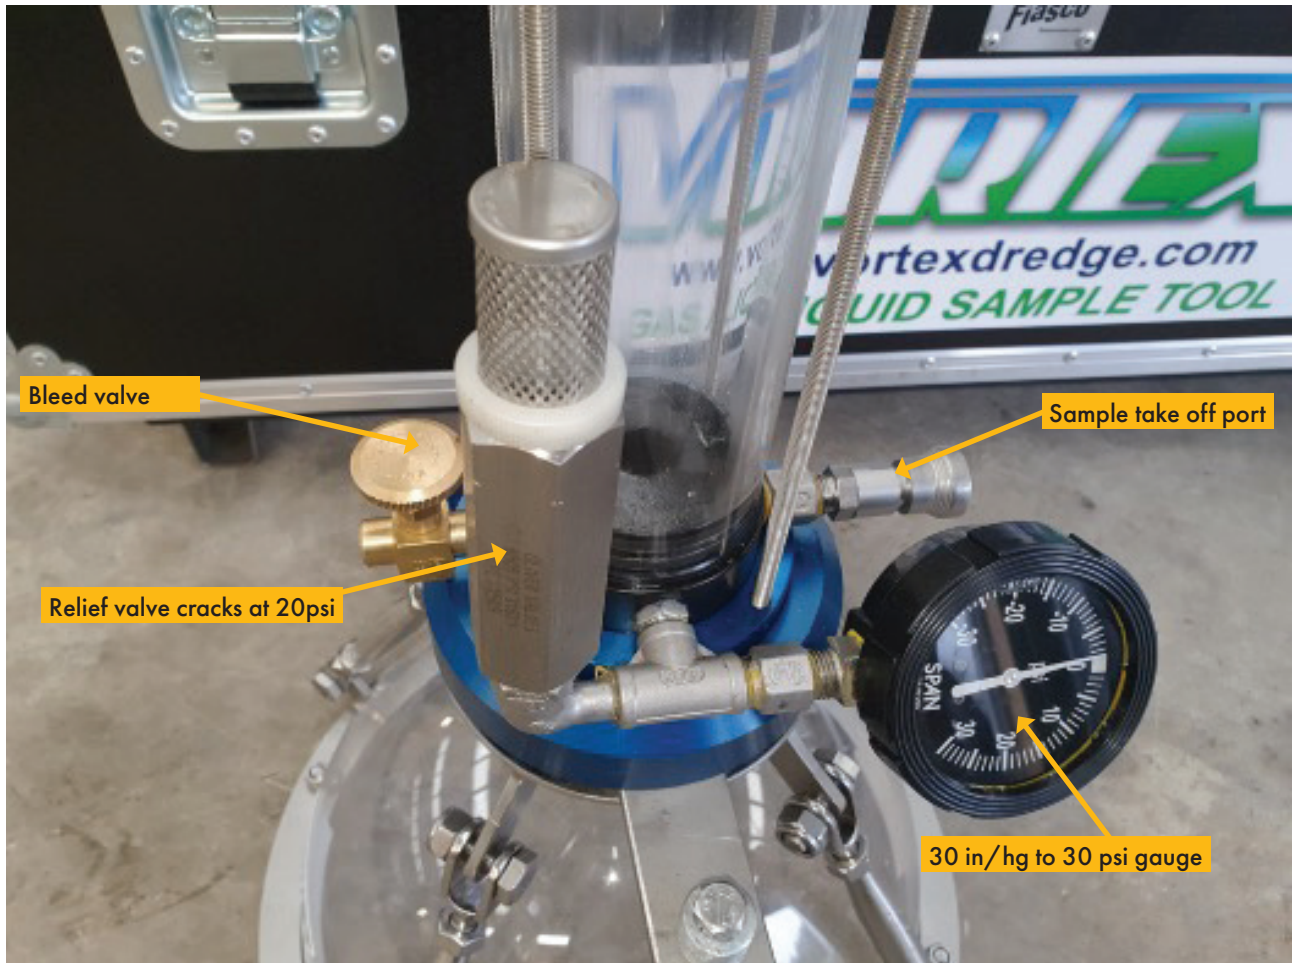

When recovering to deck, ascend at such a rate that the 0 to 30psi pressure gauge does not show over the 20 psi setting of the relief valve.

The relief valve is likely to purge excess pressure as gas expands during ascending irrespective of the rate of ascent.


# Operation Procedures

## 4.4 REMOVAL OF GAS SAMPLE ON SURFACE

STEP	PROCEDURE DESCRIPTION	CHECK
1	Recover to deck. Ascend the tool and ROV at such a rate that the 0 to 30psi pressure gauge does not show over the 20 psi setting of the relief valve. The relief valve is likely to purge excess pressure as gas expands during ascending irrespective of the rate of ascent. See 4.3 Recover to deck.	
2	Exhaust relief valve is tasked with venting any excess pressure build up in the piston due to expanding gasses on recovery to a maximum of 20 psi (0.96bar).	
3	Pull a vacuum on the sample bottle using supplied vacuum pump. Connect bottle to vacuum pump, open bottle isolation valve, pull maximum vacuum, close bottle isolation valve to seal in vacuum. See 4.4 Removal of gas sample on surface.	
4	Connect sample bottle to tool as per instructions on 4.4 Removal of gas sample on surface.  <b>NOTE:</b> Ensure area is adequately ventilated to account for any gas going over the exhaust relief valve when filling bottle. Similarly, have appropriate containment under exhaust relief valve to catch any liquids.  <b>ALWAYS</b> wear appropriate PPE and consult client for information on sample product and any appropriate safeguards.	
5	Flush the system with fresh water as per step below to resume sampling.  Flush system with hot soapy water then fresh water between sample dives if required. Stroke piston "suck" and "Blow" 4 or 5 times to flush system.  Check the piston full stroke in both directions in clear of obstructions.  Connect water hose (fresh or salt) to inlet relief valve of tool, open bleed valve CW and purge water through the bleed valve and allow water to pass over the exhaust relief valve to expel any air in the system. Close bleed valve CCW.  Launch with tool stroked to rest at full 'blow' position so it is ready to "suck" first sample.	

# Operation Procedures

## 4.4 REMOVAL OF GAS SAMPLE ON SURFACE

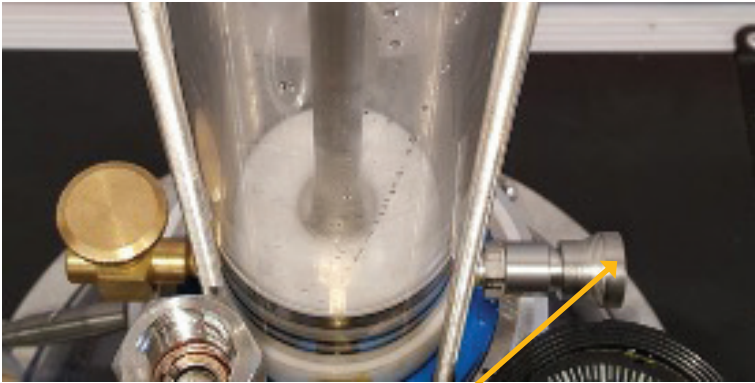

Shown bottle and sample take off port.

Pull a vacuum on the sample bottle using supplied vacuum pump.  
Connect bottle to vacuum pump.

1. Open bottle isolation valve.
2. Pull maximum vacuum
3. Close bottle isolation valve to seal in vacuum.
4. Observe and note pressure gauge reading.
5. Connect sample bottle to sample bleed off connector
6. Open bottle isolation valve.
7. Function tool to 'blow' and discharge sample product into sample bottle.
8. Close bottle isolation valve.

**NOTE:** Ensure area is adequately ventilated to account for any gas going over the exhaust relief valve when filling bottle. Similarly, have appropriate containment under exhaust relief valve to catch any liquids.

**ALWAYS** wear appropriate PPE and consult client for information on sample product and any appropriate safeguards.

# Operation Procedures

## 4.5 POST – DIVE CHECKS

STEP	PROCEDURE DESCRIPTION	CHECK
1	Check the piston full stroke in both directions in clear of obstructions.  Open bleed valve slightly CW to allow hot soapy water to flush through bleed valve	
2	Connect hose from container of hot soapy water to inlet relief valve of tool and purge soapy water through the bleed valve and allow water to pass over the exhaust relief valve to flush salt water and traces of sample from the system.  Stroke piston "suck" and "Blow" 4 or 5 times to flush system. Complete flushing with tool stroked to rest at full 'blow' position so it is ready to "suck" first sample.	
3	Check the bleed valve is closed CCW.	
4	Check mechanical connections on the tool are secure.	

# Operation Procedures

## 4.5 POST – DIVE CHECKS

POST DIVE COMMENTS		
Name:	Signature:	Date:


# Maintenance & Storage

## 5.1 STANDARD PROCEDURES

- Tool should be flushed with hot soapy water as per post dive checks.
- Allow to dry fully.
- Check operational condition of hoses.
- Visual check of tool for anything which could prohibit future operation of the tool.

## 5.2 REPLACEMENT PROCEDURES

- Contact Ashtead Technology representatives with reports of any damaged or unserviceable items.

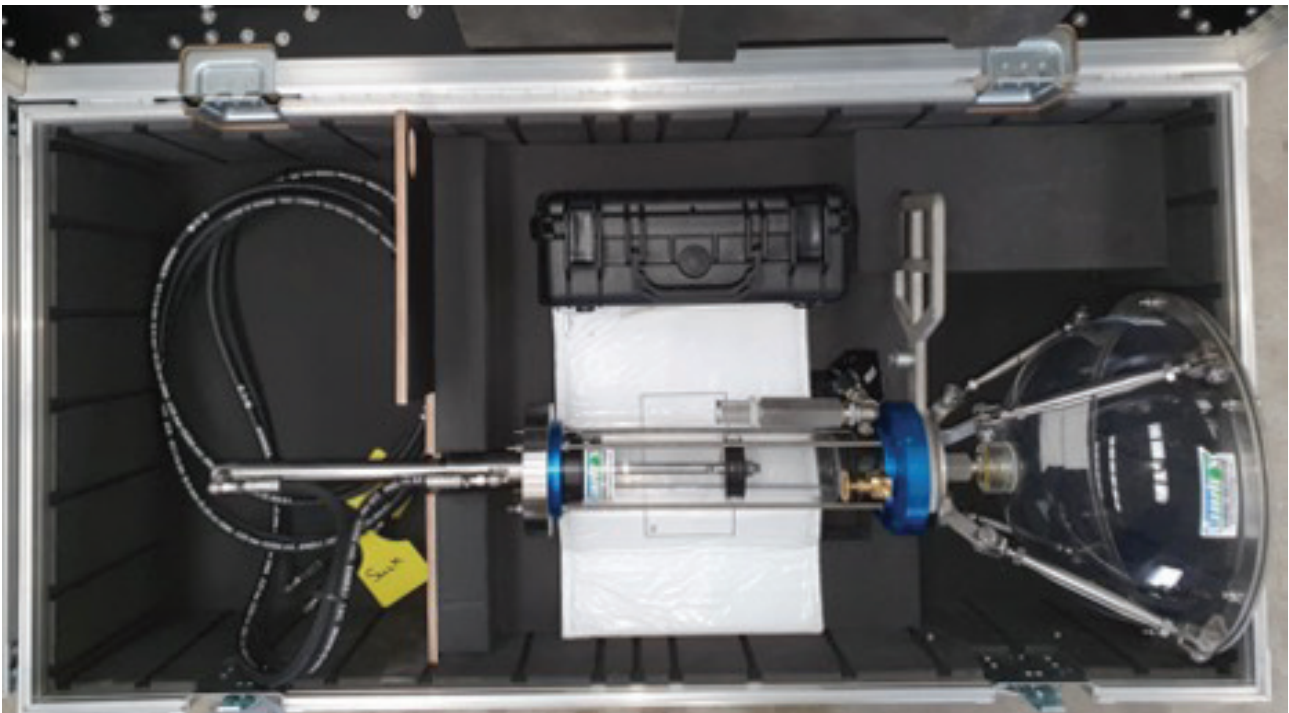

Shipping box dimensions and weight = 176 lb (66kg) L117cm x W58cm x H 48cm.

# Appendix And References

## APPENDIX I

### 6.1:1 TOOL DIMENSIONS AND WEIGHTS



Complete tool weight empty in air = 10kg (22lb)

Complete tool dimensions = 940 mm (37inch) overall height / tall x 460mm (18 inch) overall width.

# SPARES

## APPENDIX I

### 6.2 SPARES CONTENTS

1. Syringe ACRYLIC TUBE 70mm X 60mm x 280mm long
2. Item: OR053x4V75 53 x 4 Viton O-ring
3. Item: UM05006004 50 x 60 x 4 SA seal. Piston seals. (two items)
4. Cylinder seal kit.



# Appendix And References

## APPENDIX II

### BOTTLE CERTIFICATES

Part No.: 1159C-41-431	<b>ARROWHEAD INDUSTRIAL SERVICES USA, INC.</b> Compressed Gas Container Specialists 3537 S. NC 119, P.O. Box 1000 Graham, NC 27253-1000	Report No.: 2238 Sheet No.: 1 of 2
Report Date: 3/20/2013		

**CERTIFICATE OF COMPLIANCE & TEST REPORT — SEAMLESS CYLINDERS**

Manufactured for: Hoke Incorporated  
405 Centatura Court,  
Spartanburg, SC 29303

Location at: 3016 Katana Ave.  
Riverside, CA 92507

Manufactured by: Luxfer Riverside  
3016 Katana Ave.  
Riverside, CA 92507

Consigned to: Hoke Incorporated  
405 Centatura Court,  
Spartanburg, SC 29303

Location at: 3016 Katana Ave.  
Riverside, CA 92507

Quantity: 27 Size: 4.000 inches outside diameter by 9.50 inches long.

Specification: DOT-3A1800 Identifying Symbol: MS400

Serial Numbers: 647 through 673 Exceptions: none

Inspector's Mark: A Tare Weights: NO

Test Date: 3-13 Lot Number: 30

Marks stamped into the shoulder of the cylinders are: DOT-3A1800 (Ser.No) MS400 3-13 1006CC SS316

Other Marks: HOKE

These containers were made by a process of spinning both ends to form a shoulder and neck of seamless steel tubing. The cylinders were heat treated for 15 minutes @ 775° F. The material used was 316 stainless steel seamless tubing and identified by the following heat number: V01054.

The material used was verified as to chemical analysis and record thereof is attached hereto. The heat numbers were marked on the material. All material, such as plates and stainless tubing were inspected and each cylinder was inspected both before and after closing in the ends; all that was accepted was found free from seams, cracks, laminations, and other defects which and after might prove injurious to the strength of the cylinder.

The process of manufacture and heat treatment of containers was supervised and found to be efficient and satisfactory. The cylinder walls were measured and the minimum thickness noted was 0.217 inch. The outside diameter was determined by a close approximation to be 4.000 inches. The wall stress was calculated to be 32,003 pounds per square inch under an internal test pressure of 3,000 pounds per square inch.

Hydrostatic tests, flattening tests, tensile tests of material, and other tests as prescribed in DOT Specification 3A were made in the presence of the inspector and all material and containers accepted were found to be in compliance with the requirements of that specification. Records thereof are attached hereto.

I hereby certify that all of these cylinders proved satisfactory in every way and comply with the requirements of US Department of Transportation Specification 3A except as follows: none

TR221-B1  
Rev. 1, 1/17/12

Inspector, ARROWHEAD INDUSTRIAL SERVICES USA, INC.

Part No.: 1159C-41-431	<b>ARROWHEAD INDUSTRIAL SERVICES USA, INC.</b> Compressed Gas Container Specialists 3537 S. NC 119, P.O. Box 1000 Graham, NC 27253-1000	Report No.: 2238 Sheet No.: 2 of 2
Report Date: 3/20/2013		

**RECORD OF PHYSICAL TESTS OF MATERIAL FOR CYLINDERS**

Manufactured by: Luxfer Riverside

For: Hoke Incorporated

Serial numbers: 647 through 673

Exceptions:

Size: 4.000 inches outside diameter by 9.500 inches long.

Lot No.	Yield (@ .2% offset) psi	Tensile Strength psi	Elongation in 2 inches (%)	Reduction in Area (%)	FLATTENING TEST 6t
30	41,009	87,836	52.0	79	PASS
30	40,655	88,074	51.0	79	PASS

**RECORD OF CHEMICAL ANALYSIS OF MATERIAL FOR CYLINDERS**

MATERIAL TYPE: 316-stainless Steel Seamless Tubing

CAST CODE	TYPE of ANALYSIS	SERIAL No. RANGE	C	Mn	Si	P	S	Cr	Ni	Mo	Cu	Fe
V01054	mill	647 through 673	0.02	1.91	0.28	0.02	0.013	16.79	11.3	2.03	0.21	BAL

Material Manufacturer: Titan Metal Fab, Long Beach Ca, 34657, USA.

The above analyses have been verified to comply with material authorized by the specification.

Chemical analyses were made by: Stork Materials Testing and Inspection, Huntington Beach, CA 92649, USA

TR221-B1  
Rev. 1, 1/17/12

Inspector, ARROWHEAD INDUSTRIAL SERVICES USA, INC.

# Appendix And References

## APPENDIX II

### ACRYLIC TUBE PRESSURE CALCULATIONS

Programma di produzione standard			Standard production program		
Tubi Acrilici Colati Esacast®			Cast Acrylic Tubes Esacast®		
Diametro esterno mm.	Diametro interno mm.	Spessore di parete mm.	External diameter mm.	Internal diameter mm.	Wall thickness mm.
50	40-42-44	5-4-3	50	40-42-44	5-4-3
60	50-52-54	5-4-3	60	50-52-54	5-4-3
64	54-56-58	5-4-3	64	54-56-58	5-4-3
70	60-62-64	5-4-3	70	60-62-64	5-4-3
76	66-68-70	5-4-3	76	66-68-70	5-4-3
80	70-72-74	5-4-3	80	70-72-74	5-4-3
90	80-82-84	5-4-3	90	80-82-84	5-4-3
100	90-92-94	5-4-3	100	90-92-94	5-4-3
110	100-102-104	5-4-3	110	100-102-104	5-4-3
120	110-112-114	5-4-3	120	110-112-114	5-4-3
125	115-117-119	5-4-3	125	115-117-119	5-4-3
134	124-126-128	5-4-3	134	124-126-128	5-4-3
139	129-131-133	5-4-3	139	129-131-133	5-4-3
150	140-142-144	5-4-3	150	140-142-144	5-4-3
160	150-152-154	5-4-3	160	150-152-154	5-4-3
185	175-177-179	5-4-3	185	175-177-179	5-4-3
200	190-192-194	5-4-3	200	190-192-194	5-4-3
220	210-212-214	5-4-3	220	210-212-214	5-4-3
240	230-232-234	5-4-3	240	230-232-234	5-4-3
250	240-242-244	5-4-3	250	240-242-244	5-4-3
300	284-288-290-292	8-6-5-4	300	284-288-290-292	8-6-5-4
350	334-338-340-342	8-6-5-4	350	334-338-340-342	8-6-5-4
400	384-388-390-392	8-6-5-4	400	384-388-390-392	8-6-5-4
457	437-441-445-447	10-8-6-5	457	437-441-445-447	10-8-6-5
500	480-484-488-490	10-8-6-5	500	480-484-488-490	10-8-6-5

# Appendix And References

## APPENDIX II

### ACRYLIC TUBE PRESSURE CALCULATIONS CONTINUED

#### Condizioni tecniche di fornitura

##### Lunghezze standard

fino al ø esterno 250 mm.	2.000 mm.
ø est. 300 mm.	1.000/2.030/3.030 mm.
ø est. 400 mm.	1.000/2.030/2.160/3.030 mm.
ø est. 500 mm.	1.000/2.030/2.160/3.030 mm.

A richiesta per ø 200-220-240-250 è disponibile la lunghezza 3.030 mm.

##### Tolleranze sui diametri esterni

dal ø 50 mm. al ø 100 mm.	+1 / -1,5%
dal ø 110 mm. al ø 500 mm.	+1 / -1,5%

##### Tolleranze sullo spessore di parete

spessore 3 mm.	+/- 20 %
spessore 4 mm.	+/- 15 %
dallo spessore 5 mm. allo spessore 15 mm.	+/- 10 %

##### Tolleranze sulle lunghezze

+/- 1 mm.

##### Formula per il calcolo della pressione massima interna ammissibile

$$P^i = \frac{50 \times S}{D^i}$$

dove:

$P^i$  = pressione interna del tubo in atmosfere o bar (1bar=0,1 N/mm<sup>2</sup>)

$S$  = spessore del tubo in mm.

$D^i$  = diametro interno del tubo in mm.

Questa formula è valida in condizioni di test standard, e cioè ad una temperatura ambiente di 20 °C ed umidità relativa del 50%.

#### Technical delivery terms

##### Standard lengths

up to the external ø 250 mm.	2.000 mm.
ext. ø 300 mm.	1.000/2.030/3.030 mm.
ext. ø 400 mm.	1.000/2.030/2.160/3.030 mm.
ext. ø 500 mm.	1.000/2.030/2.160/3.030 mm.

On demand for ø 200-220-240-250 is available the length 3.030 mm.

##### Tolerances on the external diameter

from ø 50 mm. up to ø 100 mm.	+1 / -1,5%
from ø 110 mm. up to ø 500 mm.	+1 / -1,5%

##### Tolerances on wall thickness

thickness 3 mm.	+/- 20 %
thickness 4 mm.	+/- 15 %
from thickness 5 mm. up to thickness 15 mm.	+/- 10 %

##### Lengths tolerance

+/- 1 mm.

##### Formula for the calculation of the maximum internal allowable pressure

$$P^i = \frac{50 \times S}{D^i}$$

where:

$P^i$  = internal pressure of the tube in atmospheres or bar (1bar=0,1 N/mm<sup>2</sup>)

$S$  = thickness of the tube in mm.

$D^i$  = internal diameter of the tube in mm.

This formula is valid for standard test conditions, and it means with 20 °C room temperature and 50% of relative humidity.

17

# Appendix And References

## APPENDIX II

### ACRYLIC TUBE PRESSURE CALCULATIONS CONTINUED

#### Condizioni tecniche di fornitura

##### Lunghezze standard

fino al Ø esterno 40 mm.	2.000 mm.
oltre	2.050 mm.

##### Tolleranze sui diametri esterni

dal Ø 7 mm. al Ø 150 mm.	+/- 1 %
dal Ø 160 mm. al Ø 300 mm.	+/- 2 %

##### Tolleranze sui diametri interni

dal Ø 7 mm. al Ø 150 mm.	+/- 1,5 %
dal Ø 160 mm. al Ø 300 mm.	+/- 2,5 %

##### Tolleranze sullo spessore di parete

dal Ø 7 mm. al Ø 64 mm.	+/- 5 %
dal Ø 70 mm. al Ø 100 mm.	+/- 8 %
dal Ø 110 mm. al Ø 200 mm.	+/- 10 %
dal Ø 220 mm. al Ø 300 mm.	+/- 15 %

##### Tolleranze sulle lunghezze

+/- 1 mm.

##### Formula per il calcolo della pressione massima interna ammissibile

$$P^i = \frac{50 \times S}{D^i} \quad \text{valida per } \frac{D^o}{D^i} \leq 1,2$$

dove:

$P^i$  = pressione interna del tubo in atmosfere o bar (1bar=0,1 N/mm<sup>2</sup>)

$S$  = spessore del tubo in mm.

$D^o$  = diametro esterno del tubo in mm.

$D^i$  = diametro interno del tubo in mm.

Questa formula è valida in condizioni di test standard, e cioè ad una temperatura ambiente di 20 °C ed umidità relativa del 50%.

#### Technical delivery terms

##### Standard lengths

up to the external Ø 40 mm.	2.000 mm.
over 40 mm.	2.050 mm.

##### Tolerances on the external diameter

from Ø 7 mm. up to Ø 150 mm.	+/- 1 %
from Ø 160 mm. up to Ø 300 mm.	+/- 2 %

##### Tolerances on the internal diameter

from Ø 7 mm. up to Ø 150 mm.	+/- 1,5 %
from Ø 160 mm. up to Ø 300 mm.	+/- 2,5 %

##### Tolerances on wall thickness

from Ø 7 mm. up to Ø 64 mm.	+/- 5 %
from Ø 70 mm. up to Ø 100 mm.	+/- 8 %
from Ø 110 mm. up to Ø 200 mm.	+/- 10 %
from Ø 220 mm. up to Ø 300 mm.	+/- 15 %

##### Lengths tolerance

+/- 1 mm.

##### Formula for the calculation of the maximum internal allowable pressure

$$P^i = \frac{50 \times S}{D^i} \quad \text{valida per } \frac{D^o}{D^i} \leq 1,2$$

where:

$P^i$  = internal pressure of the tube in atmospheres or bar (1bar=0,1 N/mm<sup>2</sup>)

$S$  = thickness of the tube in mm.

$D^o$  = external diameter of the tube in mm.


$D^i$  = internal diameter of the tube in mm.

This formula is valid for standard test conditions, and it means with 20 °C room temperature and 50% of relative humidity.

# Appendix And References

## APPENDIX II


### SAMPLE BOTTLE DETAILS

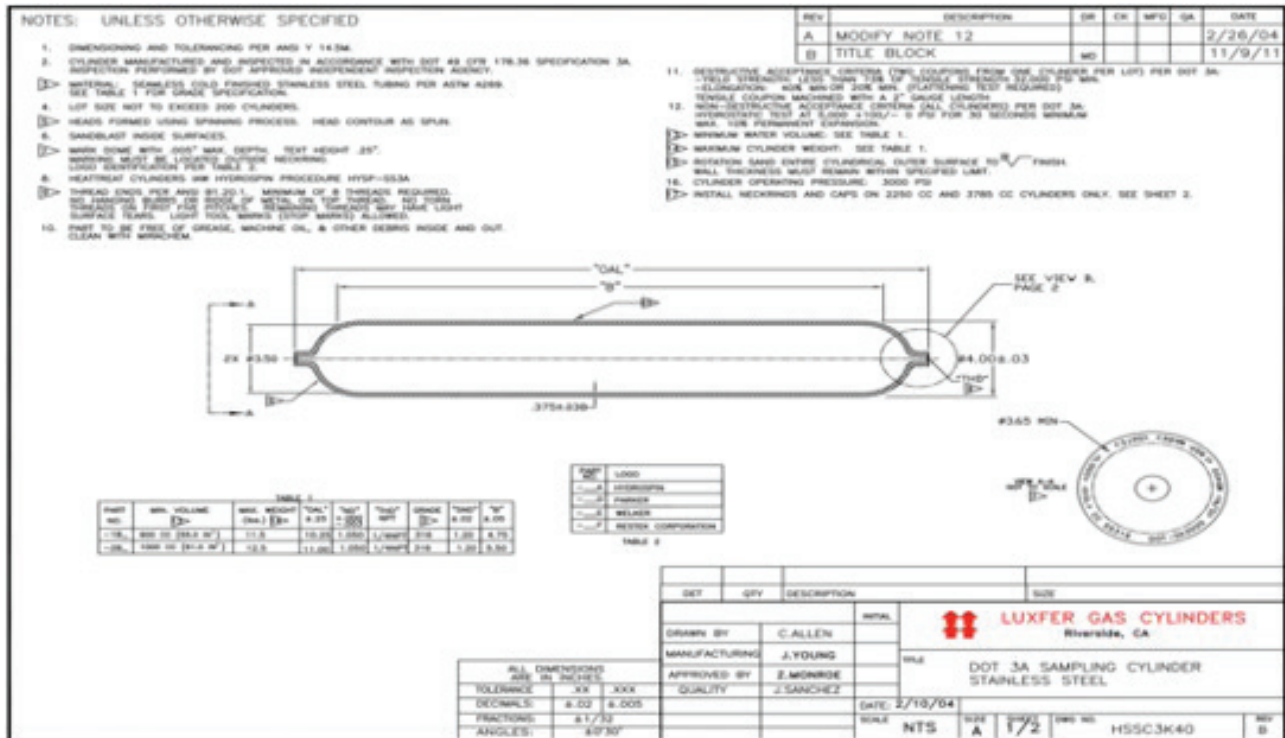

# Appendix And References

## APPENDIX II


### SAMPLE BOTTLE DETAILS

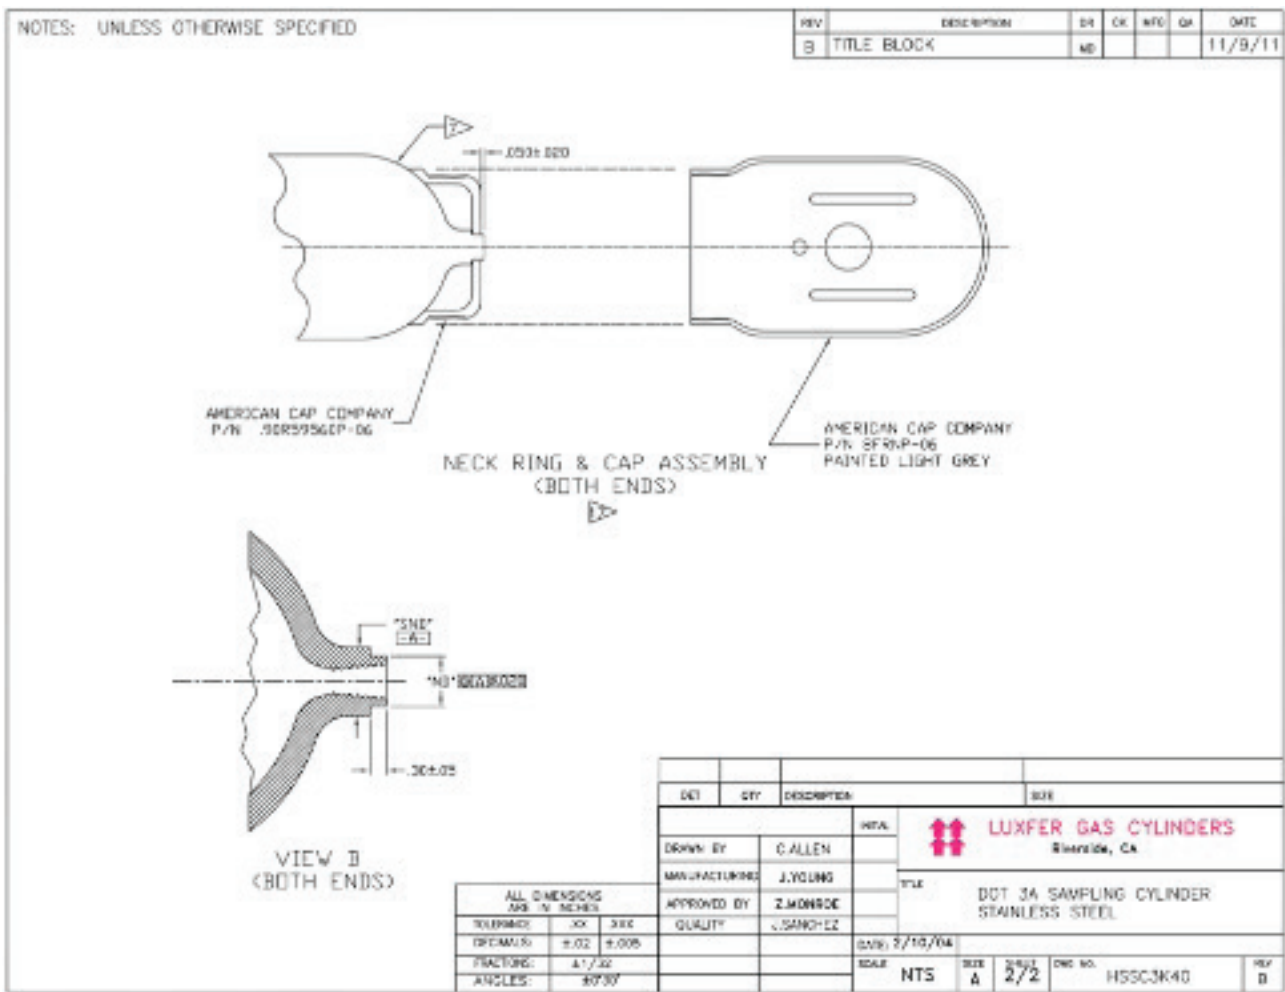

# Appendix And References

## APPENDIX II

### SAMPLE BOTTLE DETAILS

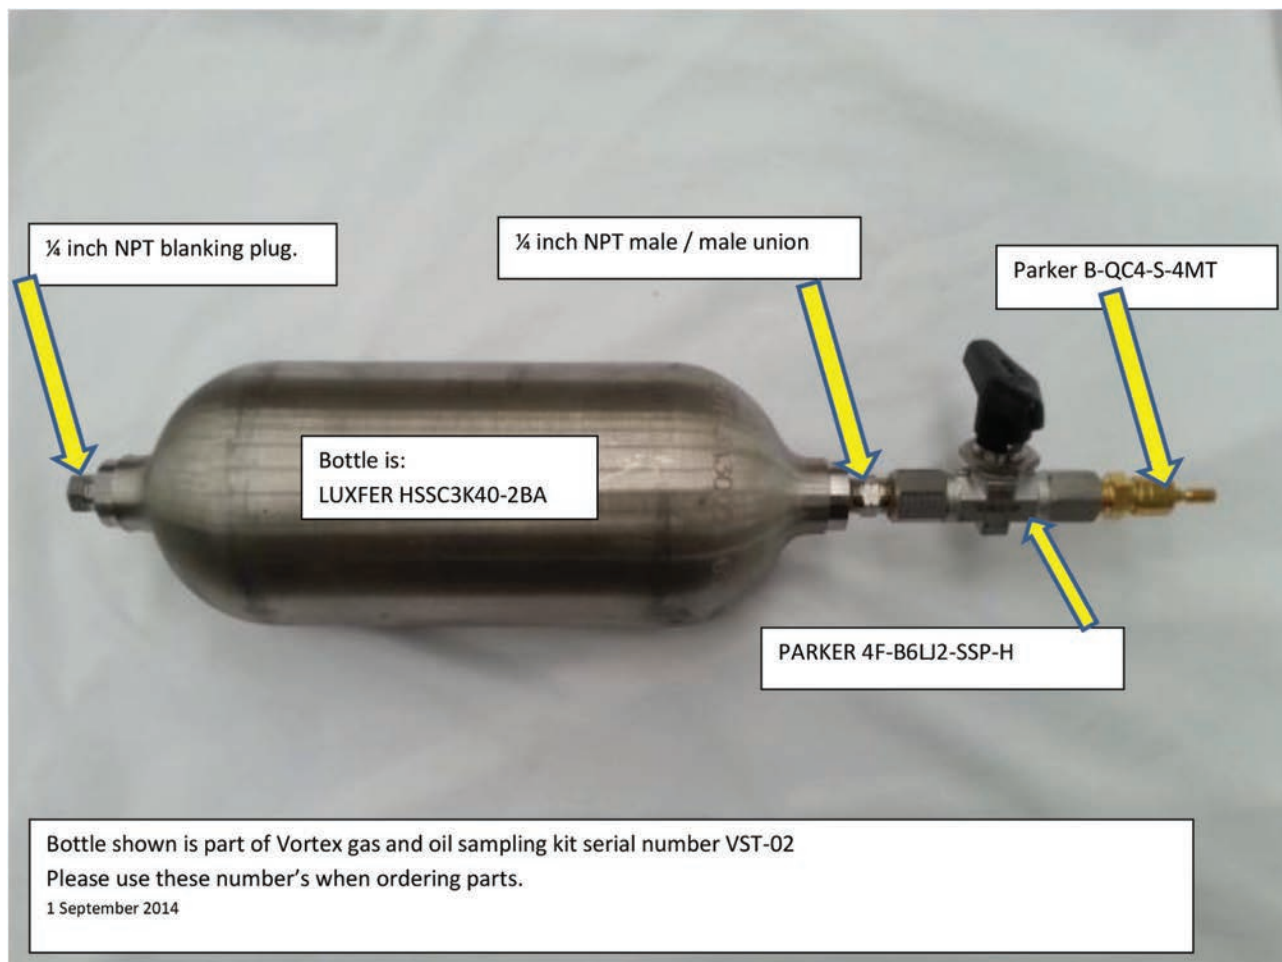

# Appendix And References

## APPENDIX II

### SAMPLE BOTTLE DETAILS

Specification	DOT-3A1800 (NACE MR0175)
Volume	1000cc (0.264 gallon)
Test date	March 2013
Material	SS 316 L
Surface coating	N/A. Bare 316 stainless steel
Test pressure	Design test pressure of 3000 psi
Working pressure	Marked service pressure 1800 psi

**It is YOUR responsibility to ensure transportation of equipment containing product and or samples complies with all relevant authorities.**

# Appendix And References

## APPENDIX II

### SAMPLE BOTTLE DETAILS

PART NUMBER	SERVICE PRESSURE	DIAMETER	LENGTH	WEIGHT	INTERNAL VOLUME	THREADS	SPECIFICATION	INCLUDED ACCESSORIES	MATERIAL
	bar	mm	mm	kg	ml				
HSSC3K1 5-3BA	207	38	221	0.6	150	.250-18 NPT	DOT-3A	-	316L Stainless
HSSC3K1 5-4BA	207	38	221	0.6	150	.375-18 NPT	DOT-3A	-	316L Stainless
HSSC30-1BA	207	76	173	2.3	300	.500-14 NPT	DOT-3A	-	316L Stainless
HSSC30-2BA	207	76	239	3.0	500	.500-14 NPT	DOT-3A	-	316L Stainless
HSSC30-3BA	207	76	417	5.6	1000	.750-14 NPT	DOT-3A		316L Stainless
HSSC3K4 0-1BA	207	102	260	5.2	900	.250-18 NPT	DOT-3A	Threaded cap & collar	316L Stainless
HSSC3K4 0-2BA	207	102	279	5.7	1000	.250-18 NPT	DOT-3A	Threaded cap & collar	316L Stainless

# Appendix And References

## APPENDIX II

### CHECK VALVE DETAILS




Product Data Sheet	Check Valve
--------------------	-------------



#### Key features

- In-line poppet type
- Allows flow in one direction only, closing when flow reverses
- Max temperature 200°C
- VITON seats (VITON 90 available for NACE, KALREZ also available if required)
- NPT female X female connections

#### General Arrangement Drawing

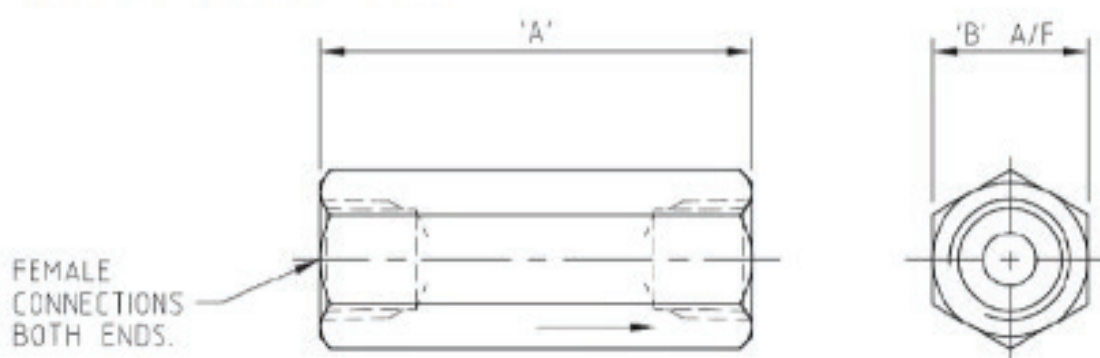


Sizes	Part No	Max Pressure	Cracking Pressure	A	B	Weight	CV (Max)
1/4"	CV25S	6,000 PSI	7 PSI	0.87"	2.31"	0.2kg	0.7
3/8"	CV38S	6,000 PSI	7 PSI	1.10"	2.50"	0.3kg	0.7
1/2"	CV50S	6,000 PSI	7 PSI	1.10"	3.06"	0.3kg	2.0
3/4"	CV75S	6,000 PSI	4 PSI	1.63"	3.63"	0.8kg	4.6
1"	CV10S	6,000 PSI	4 PSI	2.05"	4.19"	0.9kg	7.2


# Appendix And References

## APPENDIX II


### HYDRAULIC CYLINDER

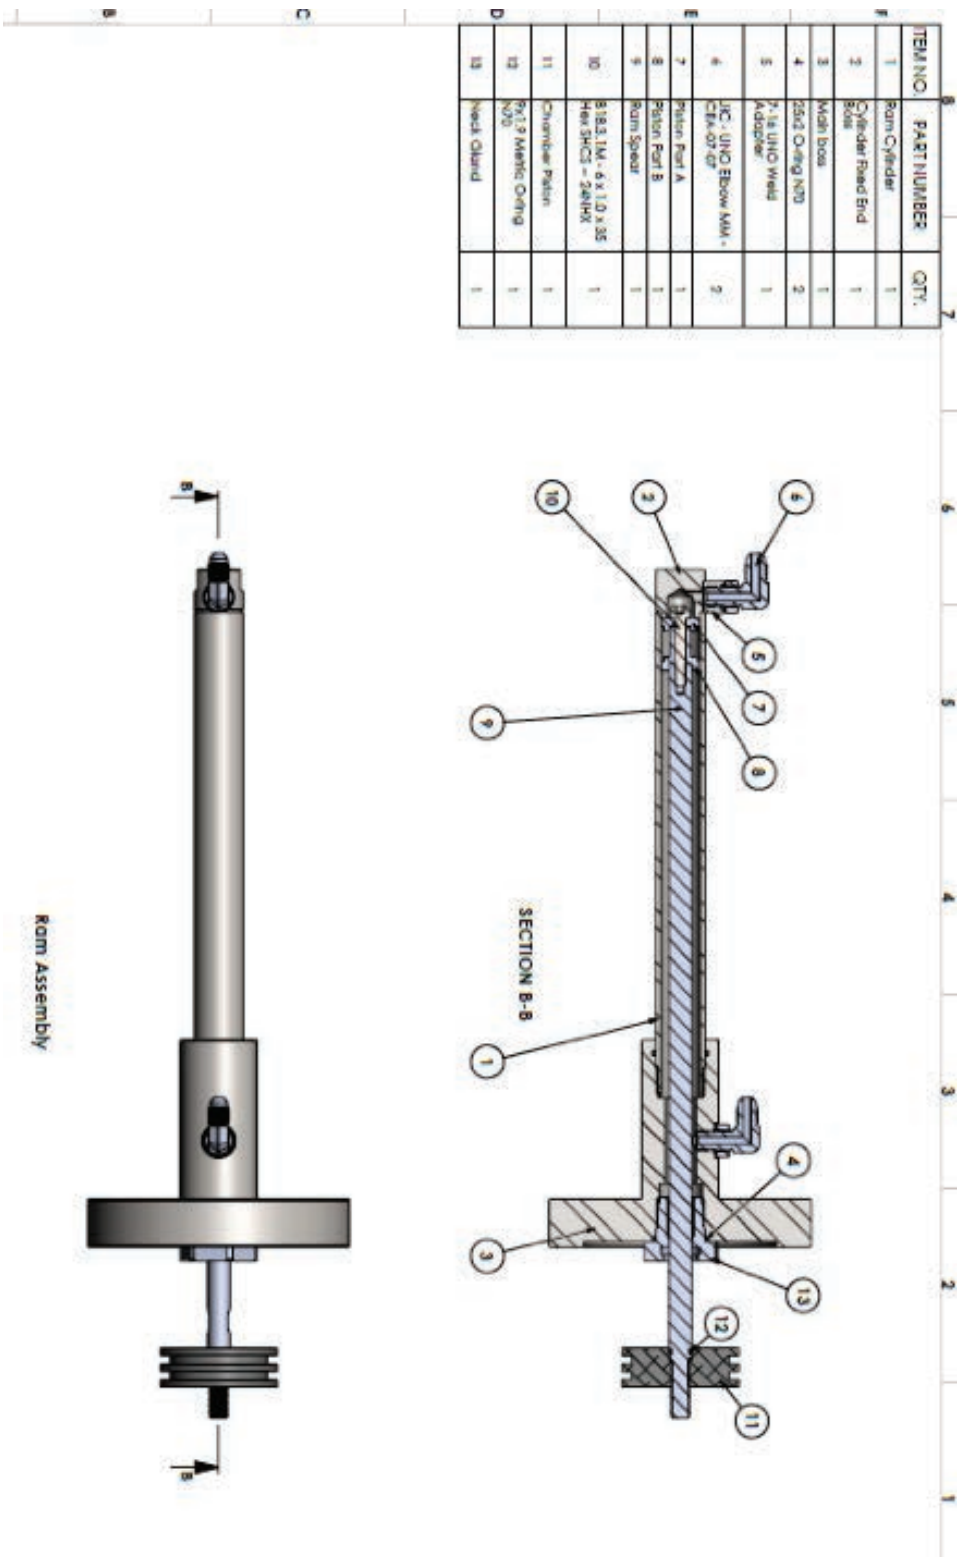

# Gas Tool Schematics

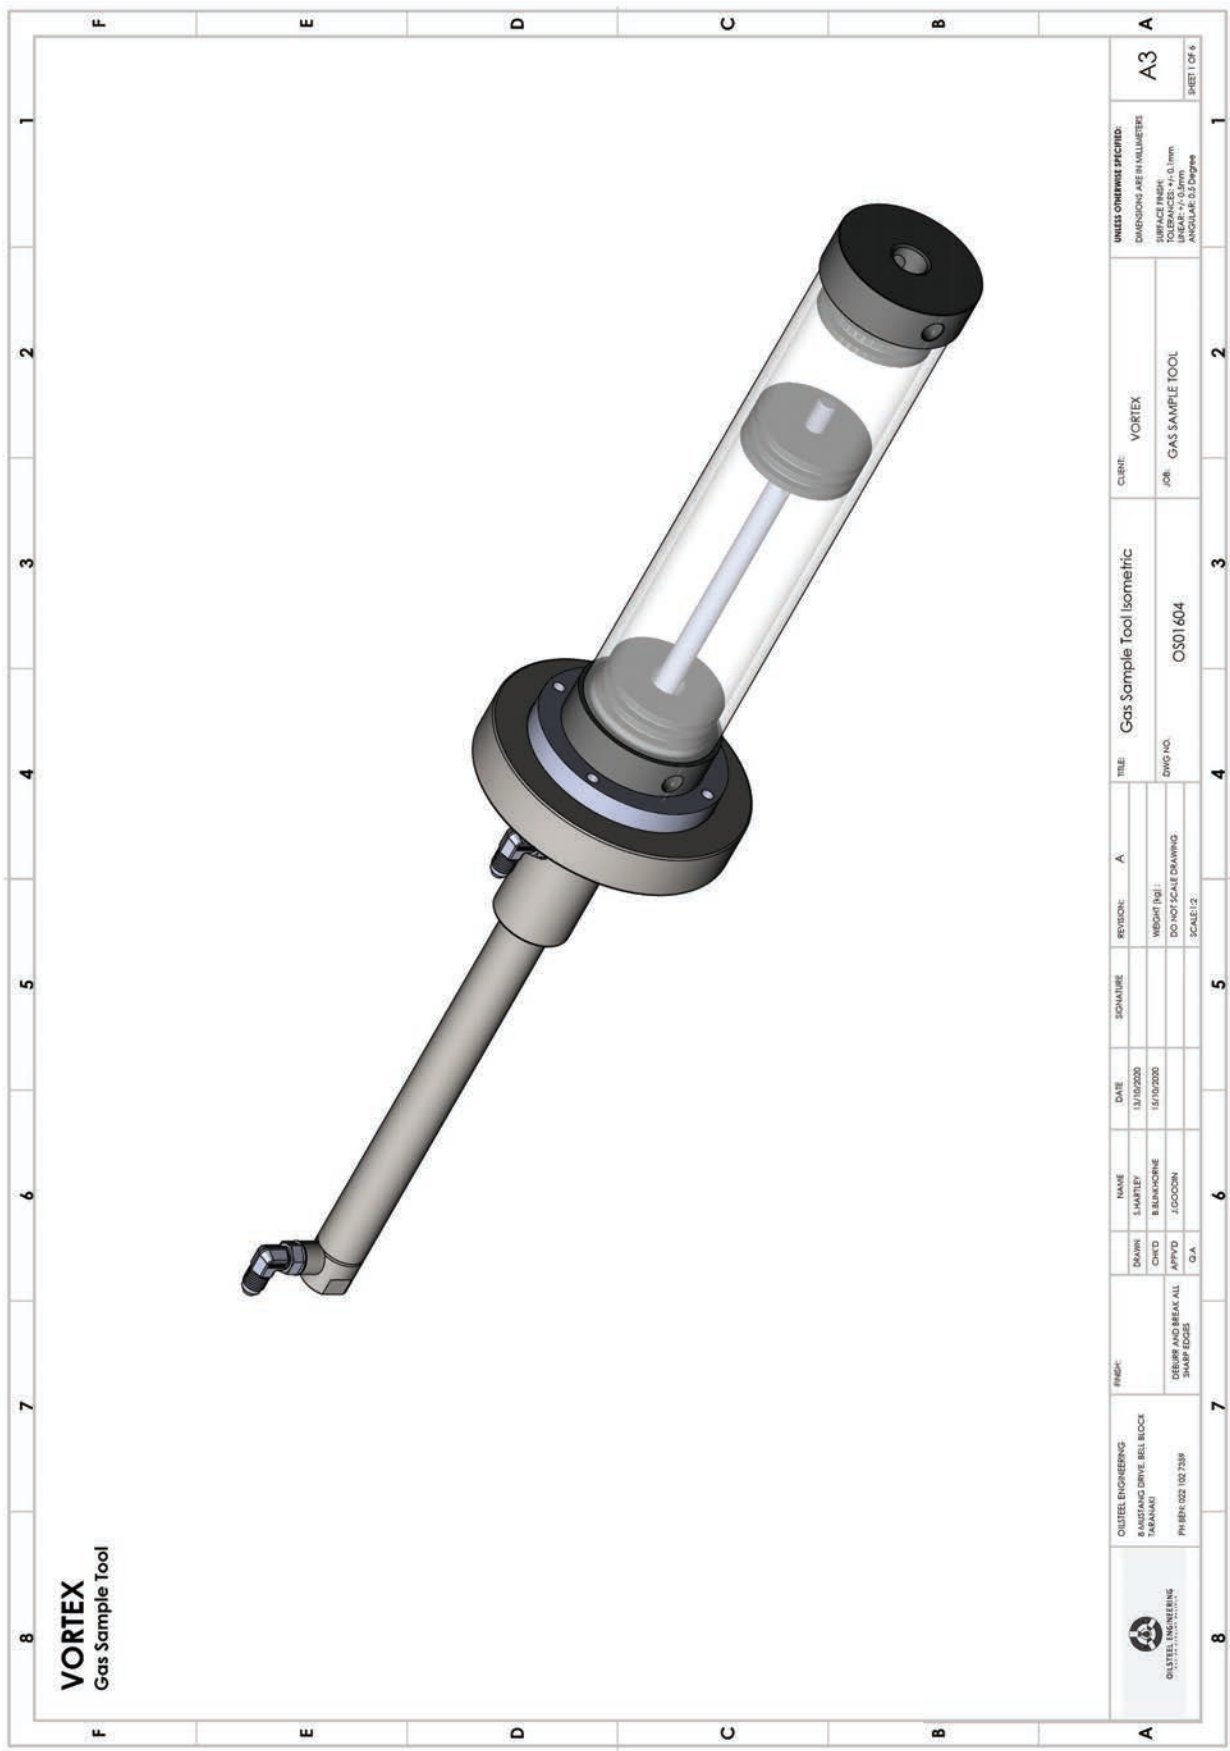

# Gas Tool Schematics

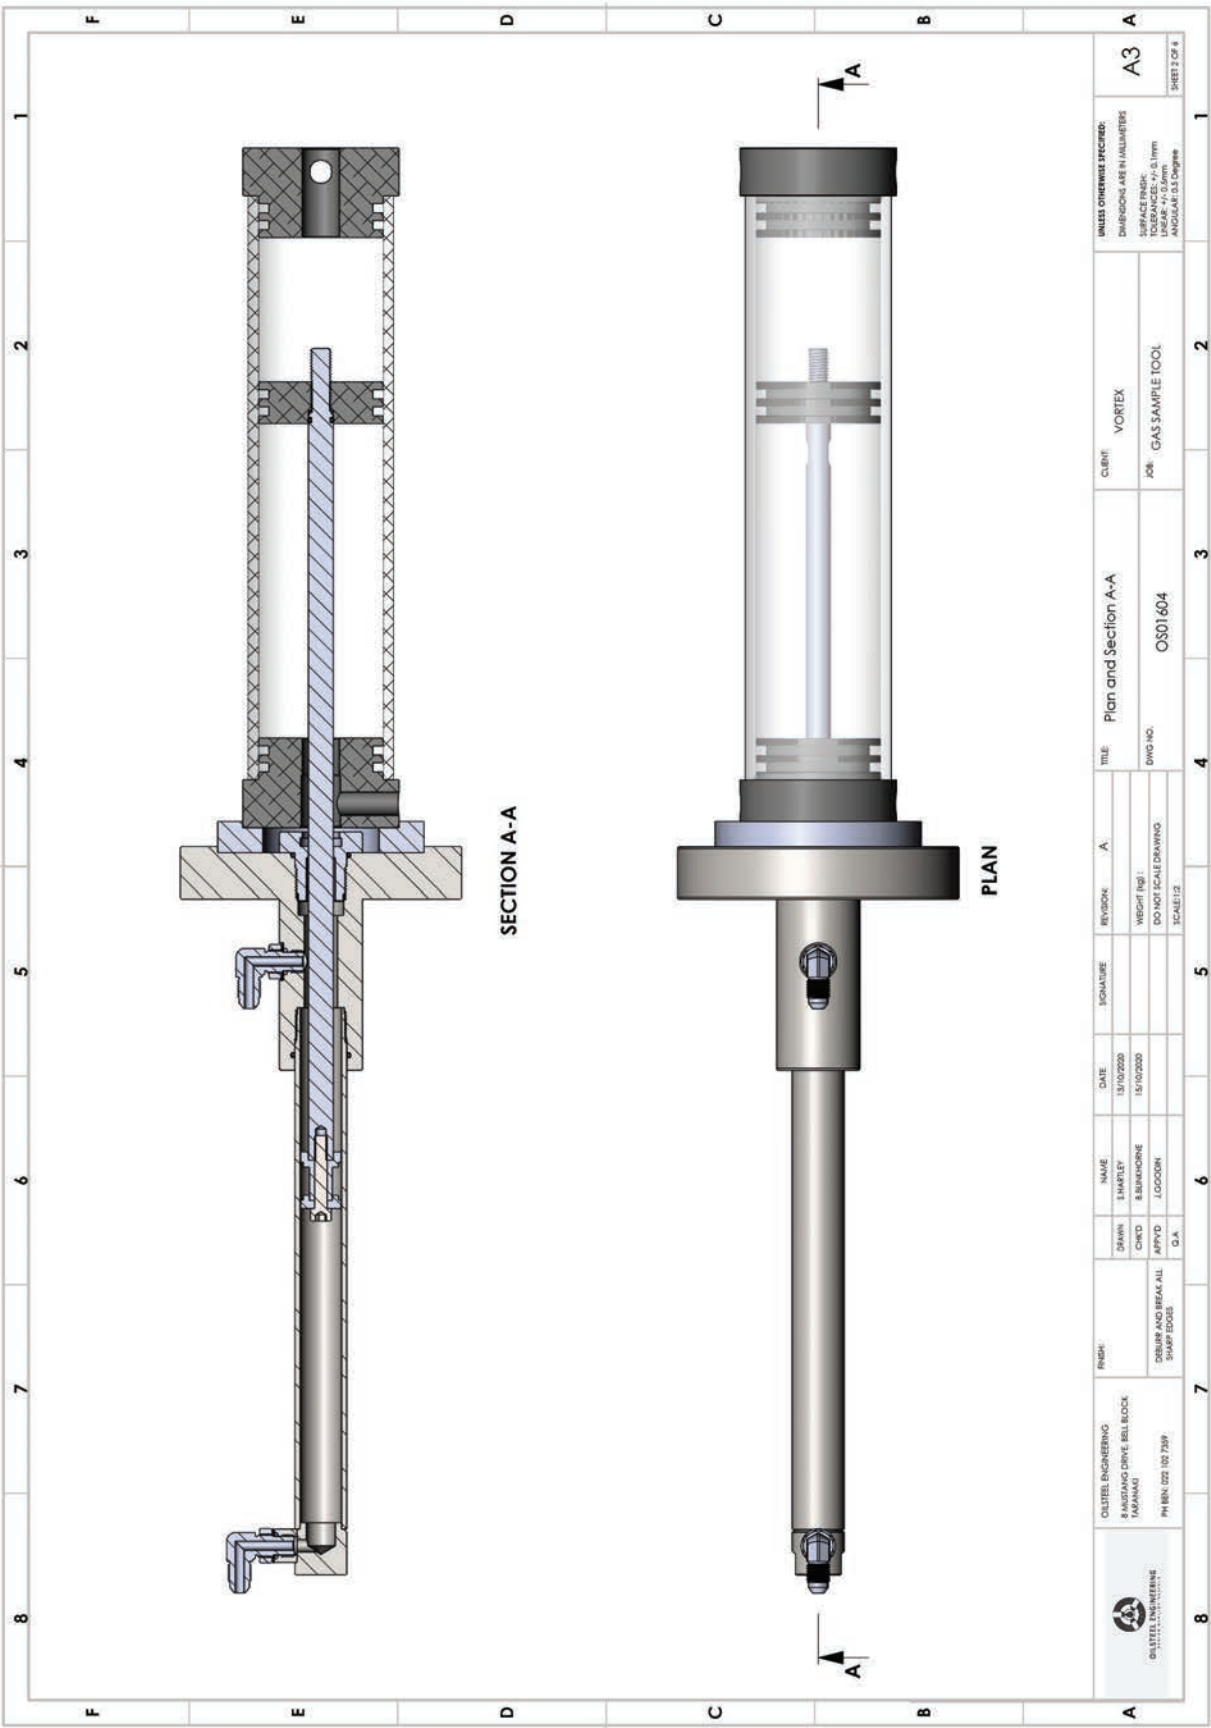


ITEM NO.	PART NUMBER	QTY.
1	Ram Cylinder	1
2	Cylinder Fixed End Boss	1
3	Main boss	1
4	25x2 O-ring N70	2
5	7-16 UNO Weld Adapter	1
6	JIC - UNO Elbow MM - CEA-07-07	2
7	Piston Part A	1
8	Piston Part B	1
9	Ram Spear	1
10	B18.31M - 6 x 1.0 x 35 Hex SHCS - 24NPK	1
11	Chamber Piston	1
12	9x1.9 Metric O-ring N70	1
13	Neck Gland	1

REV	DATE	BY	CHKD	APP'D	DESCRIPTION
1	13/10/2020	S. K. SHARTEY			
2	13/10/2020	S. K. SHARTEY			


UNLESS OTHERWISE SPECIFIED:  
DIMENSIONS ARE IN MILLIMETERS  
SURFACE FINISH:  
TOLERANCES: ±0.1mm  
UNLESS NOTED OTHERWISE  
MATERIALS: AS SPECIFIED

UNLESS OTHERWISE SPECIFIED:  
DIMENSIONS ARE IN MILLIMETERS  
SURFACE FINISH:  
TOLERANCES: ±0.1mm  
UNLESS NOTED OTHERWISE  
MATERIALS: AS SPECIFIED

# Gas Tool Schematics

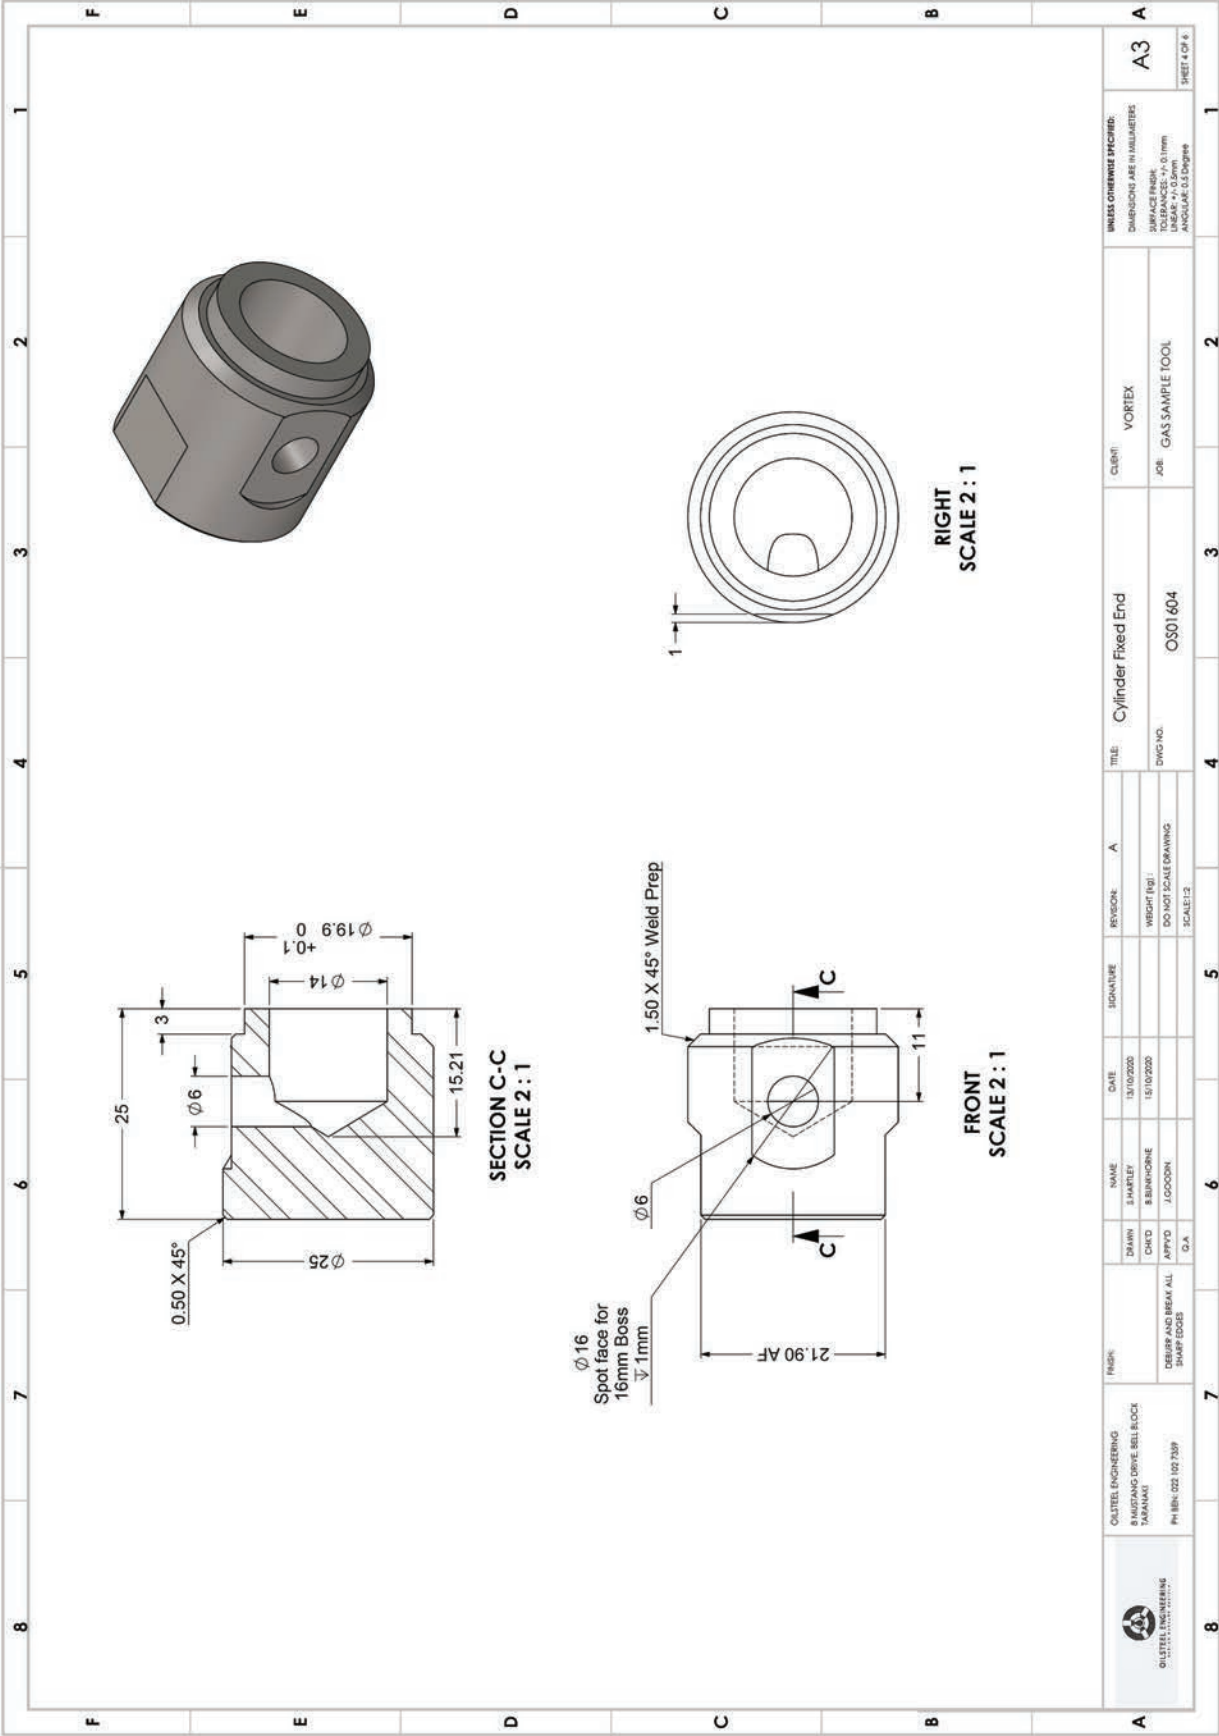

# Gas Tool Schematics

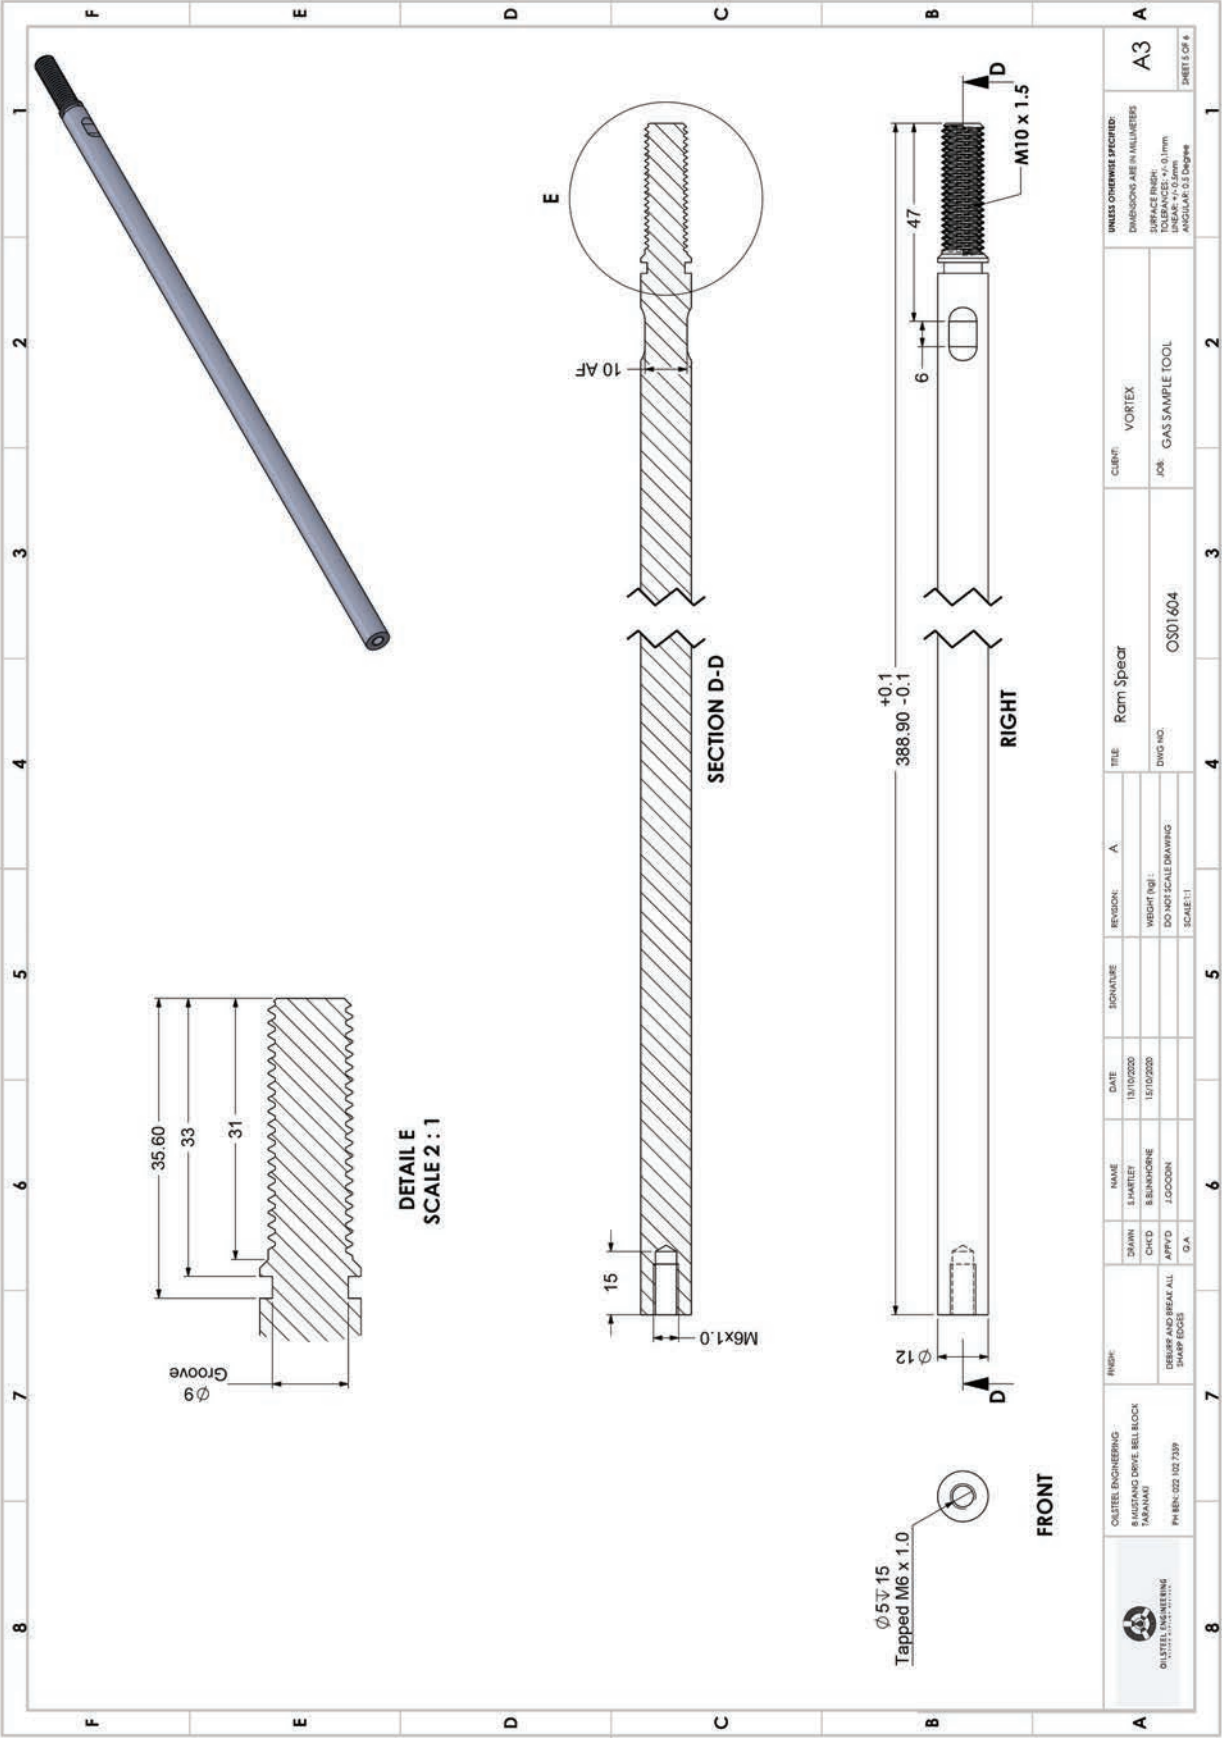

**RAM NECK GLAND**

**SECTION G-G  
SCALE 2 : 1**

**VIEW SCALE 2 : 1**

**VIEW SCALE 2 : 1**

NAME	DATE	SIGNATURE	REVISION	TITLE	CUSTOMER	UNLESS OTHERWISE SPECIFIED: DIMENSIONS ARE IN MILLIMETERS TOLERANCES - FRACTIONS - DECIMALS - ANGLES LINEAR +0.5mm ANGULAR ±0.5 Degree
NAME	DATE	SIGNATURE	REVISION	TITLE	CUSTOMER	
DRAWN	CHKD		WEIGHT Pkg :	JOB		
DESIGNED BY	APP'D		DO NOT SCALE DRAWING	DWG NO.		
SHARP EDGES	G.A.		SCALE IT	O/SO 604		
OLSTEEL ENGINEERING # EASTANG DRIVE, BELL BLOCK TARANAKI	FINISH					A3
PH EN 022 02 733P						SHEET 6 OF 6

# Contacts



## JOE GOODIN

MANAGING DIRECTOR

VORTEX International Ltd

27 Parrs Road, RD1, New Plymouth, New Zealand

Tel/Fax: +64 (6) 753 8102, Mobile: + 64 (0) 27 688 5372

Email: [joe@vortexdredge.com](mailto:joe@vortexdredge.com)

Website: [vortexdredge.com](http://vortexdredge.com)



IN ASSOCIATION WITH ASHTEAD TECHNOLOGY:

## ABERDEEN

Ashtead Technology Ltd

Ashtead House, Discovery Drive, Arnhall Business Park,  
Westhill, Aberdeenshire AB32 6FG

Tel: +44 (0) 1224 771888,

Email: [aberdeen@ashtead-technology.com](mailto:aberdeen@ashtead-technology.com)

## SINGAPORE

Ashtead Technology (S.E.A) Pte Ltd

Loyang Offshore Supply Base, 25 Loyang Crescent,  
Block 302, Unit 02-12 TOPS Ave 3, PO Box 5157,  
SINGAPORE 508988

Tel: +65 6545 9350,

Email: [singapore@ashtead-technology.com](mailto:singapore@ashtead-technology.com)

## HOUSTON

Ashtead Technology Offshore Inc

19407 Park Row, Suite 170, Houston, TX 77084, U.S.A

Tel: +1 281 398 9533,

Email: [houston@ashtead-technology.com](mailto:houston@ashtead-technology.com)

## SCOPE ENGINEERING

(Ashtead Technology Agent)

Scope Engineering (WA) Pty Ltd

35 Stuart Drive, Henderson, Western Australia 6166

T: +61 8 6498 9642 F: +61 8 6498 9584,

Email: [Perth@ashtead-technology.com](mailto:Perth@ashtead-technology.com)

## INNOVA AS

P.O. Box 390 Forus, 4067 Stavanger

Phone: +47 51 96 17 00

Fax: +47 51 96 17 01

Email: [post@innova.no](mailto:post@innova.no)

## TES SURVEY EQUIPMENT SERVICES LLC

PO Box 128256

Abu Dhabi, UAE

Tel: + 971 2 650 7710

Fax: +971 2 650 7200

Email: [info@tesme.com](mailto:info@tesme.com)



[vortexdredge.com](http://vortexdredge.com)